

HIGH VOLTAGE POWER SUPPLY HiVo
USER MANUAL

Rel. 01.01.0003
(Hardware code: HiVo-N)



Information provided in this manual is property of IPSES S.r.l. and must be considered and treated as confidential. This publication can only be reproduced, transmitted, transcribed or translated into any human or computer language with the written consent of IPSES S.r.l.

Information in this documentation has been carefully checked and is believed to be accurate as of the date of publication; however, no responsibility is assumed of inaccuracies. IPSES will not be liable for any consequential or incidental damages arising from reliance on the accuracy of this documentation.

Information contained in this manual is subject to change without notice and does not represent a commitment on the part of IPSES. The design of this instrument is subject to continue development and improvement. Consequently, the equipment associated to this document may incorporate minor changes in detail from the information hereafter provided.

All brand or product names are trademarks or registered trademarks of their respective holders.

This manual in English is the original version.

Printed in Italy

Copyright © 2009-2016 IPSES S.r.l.

All rights reserved.

GUARANTEE

IPSES warrants to the end-user in accordance with the following provisions that its branded hardware products, purchased by the end-user from IPSES company or an authorized IPSES distributor will be free from defects in materials, workmanship and design affecting normal use, for a period of one year as of the original purchase date. Products for which proper claims are made will, at IPSES's option, be repaired or replaced at IPSES's expense¹.

Exclusions

This Guarantee does not apply to defects resulting from: improper or inadequate installation, use or maintenance; actions or modifications by unauthorized third parties or the end-user; accidental or wilful damage or normal wear and tear.

Making a claim

Claims must be made by contacting IPSES office within the guarantee period.
Please, contact:

IPSES S.r.l. - Via Suor Lazzarotto, 10 - 20020 Cesate (MI) Italy
Tel. (+39) 02 39449519 – (+39) 02 320629547
Fax (+39) 02 700403170
<http://www.ipses.com> - e-mail: support@ipses.com

Limitation and Statutory Rights

IPSES makes no other warranty, guarantee or like statement other than as explicitly stated above and this Guarantee is given in place of all other guarantees whatsoever, to the fullest extent permitted by law. In the absence of applicable legislation, this Guarantee will be the end-user's sole and exclusive remedy against IPSES.

General Provisions

IPSES makes no express warranties or conditions beyond those stated in this warranty statement. IPSES disclaims all other warranties and conditions, express or implied, including without limitation implied warranties and conditions of merchantability and fitness for a particular purpose.

IPSES's responsibility for malfunctions and defects in hardware is limited to repair and replacement as set forth in this warranty statement.

IPSES does not accept liability beyond the remedies set forth in this warranty statement or liability for incidental or consequential damages, including without limitation any liability for products not being available for use or for lost data or software.

¹ With the exclusion of shipping costs for and from IPSES's development office.

WARNING!
ELECTRICAL DEVICES COULD DAMAGE EQUIPMENT OR PROPERTY OR CAUSE PERSONAL INJURY

This guide contains instructions and technical features of the HIGH VOLTAGE POWER SUPPLY HiVo.

Read with attention before attempting to install.

It is the responsibility of the technician to undertake all the safety rules provided by the law during the installation and the use of this device.

For any information which is not contained in this guide, please contact:

IPSES S.r.l. - Via Suor Lazzarotto, 10 - 20020 Cesate (MI) Italy

Tel. (+39) 02 39449519 – (+39) 02 320629547

Fax (+39) 02 700403170

<http://www.ipses.com> - e-mail: support@ipses.com

TABLE OF CONTENTS

REVISION HISTORY	6
GENERAL FEATURES.....	7
FRONT PANEL.....	7
REAR PANEL	8
INSTALLATION INSTRUCTIONS.....	9
TECHNICAL FEATURES.....	9
MANTEINANCE	10
OTHER AVAILABLE MODELS	10
PRODUCT CODE	10
CONTACTS	11
SUPPORT INFORMATION.....	12
PROBLEM REPORT.....	12
ENGINEERING PROBLEM REPORT.....	13

REVISION HISTORY

Manual revision history

Revision/ Date	Change description	Author
01.00.0000 January, 2004	First version Released	Mancuso C.
01.01.0000 February, 2008	Second version, according to new upgrade	Pizzocolo / Barbera
01.01.0001 June, 2011	Minor changes	Mancuso C.
01.01.0002 June, 2015	Update document layout	Bottaccioli M.
01.01.0003 August, 2016	Added ISO 9001:20015 logo	Bottaccioli M.

GENERAL FEATURES

HiVo is a device especially conceived to provide an adjustable elevated voltage between 320V and 1.995V, with a maximum current up to 2 mA.


For this **HiVo** is the right instrument to power photomultipliers and to polarize any device needing high voltage and low current supply.

HiVo is equipped with a **3.5 digit LCD display** showing the output voltage.

A **10-turn potentiometer** sets the voltage and assures precision and stability..

Besides, **HiVo** is equipped with an **interlock circuit** which can be used to stop the power supply if the load is not correctly connected or the photomultiplier is not correctly placed.

FRONT PANEL

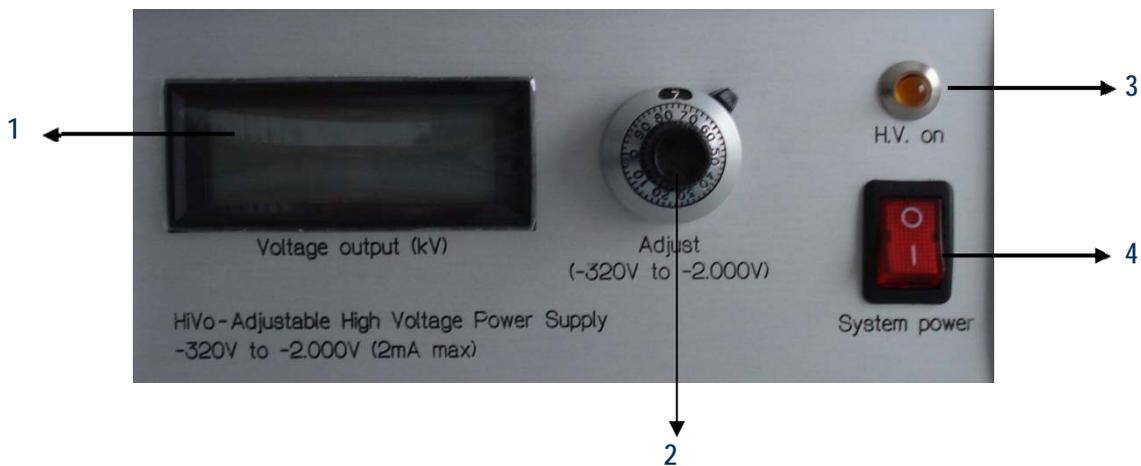

Elements present on the front panel:

1. **3.5 digit LCD display (*Voltage output*)** showing the output voltage set by the user. This value may range approximately from 320V to 1.995V.
2. **10-turn potentiometer (*Adjust*)** to set the output voltage.
3. **Yellow LED (*H.V. on*)**: when this led is lit, the power supply exit is enabled.
4. **System power switch with indicative light (*System power*)**.

CAUTION!

When the yellow LED "H.V. on" is lit, there is a high voltage on the output connector and on the connected devices.

Warning: this voltage could damage equipment or cause personal injury.

REAR PANEL



Elements present on the rear panel:

1. **AC line input** equipped with a fuse. The input voltage value will depend on the chosen model of power supply.
2. **Yellow LED (*H.V. on*)**: when this led is lit, the power supply exit is enable.
3. **SHV high voltage coaxial connector (*H.V. out*)** which the load must be connected to.
4. **Interlock connector (*Interlock H.V.*)**: it will enable the power supply exit when it is in short circuit.

CAUTION!

The load must be connected to the power supply through a **high voltage cable equipped with a SHV high voltage coaxial connector**: any other connection system could damage equipment or cause personal injury. We recommend to purchase a connection cable produced by IPSES.

INSTALLATION INSTRUCTIONS

HiVo must be used and kept dry in cool conditions.

Before plugging HiVo to the electric line, we strongly recommend to connect it to the load, so that the SHV coaxial connector will not touch accidentally anything. The interlock connector must be connected immediately after the connection of the load.

Before switching on the device, we recommend to completely turn the potentiometer (Adjust) anticlockwise, so that the unit will yield the minimum voltage (about 320V).

After that, it is possible to switch on the device through the power switch: if all the connections have properly been executed, then the LCD display will show the output voltage value and the yellow LED "H.V. on" will light.



TECHNICAL FEATURES

- **Input voltage:** 230Vac 50/60Hz (other voltage available on request)
- **Output voltage:** adjustable between -320V and -1.995V (or, on request, between +320V and +2.000V).
- **Output current:** 2mA maximum
- **Output connector:** coaxial high voltage (SHV)
- **Ripple Noise (peak to peak):** less than 0.001%
- **Rise time (from 0% to 99%) :** 150ms typ.
- **Temperature coefficient:** +/- 0,01 %/°C typ.
- **Range of operating temperature:** from 0 up to 40°C (from 32 up to 104°F)
- **Range of storage temperature:** from -20 up to +60°C (from -4 up to 140°F)
- **Activation interlock for the high voltage output switch on.**
- **Size:** about 200 x 100 x 130 mm (7.9 x 3.9 x 5.1 inches)

MANTEINANCE

Wipe the outside of the device with a clean, dry cloth. Never use harsh or abrasive cleaners or organic solvents on the device or any of its parts.

To clean the LCD display:

1. Blow gently on the LCD display to remove dust and dirt.
2. Moisten the LCD display by lightly breathing on it.
3. Wipe the LCD display gently with a soft, lint-free cloth or an untreated lens-cleaning tissue.

Do not wipe the LCD display with chemically treated eyeglass lens tissue. It may scratch the screen.

Always follow basic safety precautions. To avoid damaging your device, **DO NOT** expose it to moisture and extreme temperatures. **DO NOT** allow any chemicals to come into contact with the surface of HiVo. **NEVER** disassemble or touch the inside of the device. For any maintenance problem, please contact **IPSES** Operations Office.

OTHER AVAILABLE MODELS

IPSES can realize customized versions of HiVo device to answer to any client demands.

Particularly, it is possible to have HiVo work with any power supply voltage, with positive or negative output voltage, with output current sensing and current display.

Thanks to its customized planning, Hivo is a device which can serve our clients' needs to the best at reasonable prices.

To get more news visit the website <http://www.ipses.com>.

PRODUCT CODE

Code	Description
HiVo	Negative high voltage power supply (-1.995V, 2mA)
HiVo+2000	Positive high voltage power supply (+1.995V, 2mA)
Interlock Cable	Interlock Cable
H.V. Cable	H.V. Cable

CONTACTS

IPSES S.r.l. conceives, projects and markets electronic and scientific instruments. The customized planning of our devices allows us to answer specific necessities for customers asking for embedded systems. **IPSES** clients enjoy access to a dedicated project engineering team, available as needed.

Our pool consists of highly competent professionals whose experience in this field is extremely strong. Thanks to constant updating and technical development, **IPSES** is a leading company, combining the dynamism of a young group into the competence and reliability of a qualified staff.

IPSES S.r.l.

Research and development office:

Via Suor Lazzarotto, 10
20020 Cesate (MI)
Italy

tel. (+39) 02 39449519 - (+39) 02 320629547

fax (+39) 02 700403170

e-mail: info@ipses.com

<http://www.ipses.com>



SUPPORT INFORMATION

The customer is at liberty to contact the relevant engineer at IPSES S.r.l. directly.

Telephone	:	(+39) 02 39449519 (+39) 02 320629547
Fax	:	(+39) 02 700403170
Email	:	support@ipses.com

PROBLEM REPORT

The next page is a standard template used for reporting system problems. It can be copied and send as a fax. Alternative bugs may be reported by emails, in this case please insure that the mail contains similar information listed in the *Engineering Problem Report* form.

ENGINEERING PROBLEM REPORT

Problem describer

Name		IPSES s.r.l. Via Suor Lazzarotto, 10 Cesate (MI) Italy Fax (+39) 02 700403170 e-mail support@ipses.com
Company		
Date	Tel.	

Product

Name	Version	Serial No.
------	---------	------------

Report Type (bug, change request or technical problem)

Major bug	<input type="checkbox"/>	Urgency:	
Minor bug	<input type="checkbox"/>	High	<input type="checkbox"/>
Change request	<input type="checkbox"/>	Medium	<input type="checkbox"/>
Technical problem	<input type="checkbox"/>	Low	<input type="checkbox"/>

Problem Description

Reproduction of Problem

IPSES s.r.l. Action notes

Received by	Date	Report No.	Action
-------------	------	------------	--------

(Product code HiVo-N Rel. 01.01.0003)

IPSES S.r.l.

Via Suor Lazzarotto, 10
20020 Cesate (MI) - ITALY
Tel. (+39) 02 39449519 – (+39) 02 320629547
Fax (+39) 02 700403170
e-mail: info@ipses.com
support@ipses.com